



60W Reliable Dual Output Medical Grade

RPD-60 series



■ Features

- 4"×2" compact size
- Medical safety approved (2 x MOPP) according to ANSI/AAMI ES60601-1 and IEC/BS EN/EN60601-1
- Suitable for BF application with appropriate system consideration
- Cooling by free air convection
- EMI class B for class I configuration
- Extremely low leakage current
- Protections: Short circuit / Overload / Over voltage
- 3 years warranty

■ Applications


- Oral irrigator
- Hemodialysis machine
- Medical computer monitors
- Sleep apnea devices

■ Description

RPD-60 is a 60W highly reliable green PCB type medical power supply with a high power density on the 4" by 2" footprint. It accepts 90~264VAC input and offers dual output voltages .

RPD-60 is able to be used for Class I (with FG) system design. The extremely low leakage current is less than 150μA. In addition, it conforms to international medical regulations (2*MOPP) and EMC BS EN/EN55011.

■ Model Encoding

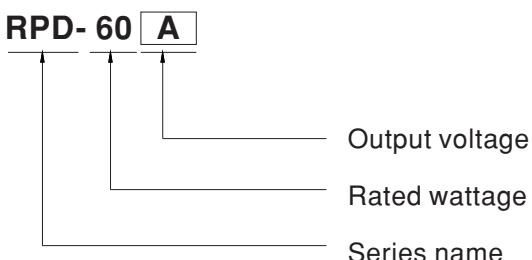



60W Reliable Dual Output Medical Grade

RPD-60 series

SPECIFICATION


MODEL	RPD-60A		RPD-60B				
OUTPUT	OUTPUT NUMBER	CH1	CH2	CH1			
	DC VOLTAGE	5V	12V	5V			
	RATED CURRENT	5A	2A	3.5A			
	CURRENT RANGE	0.5 ~ 5.5A	0.1 ~ 2.2A	0.5 ~ 3.85A			
	RATED POWER	49W		53.5W			
	PEAK LOAD(10sec.) Note.2	53.9W		58.85W			
	RIPLLE & NOISE (max.) Note.3	80mVp-p	80mVp-p	80mVp-p			
	VOLTAGE TOLERANCE Note.4	+3,-2%	±6.0%	+3,-2%			
	LINE REGULATION	±0.5%	±1.0%	±0.5%			
	LOAD REGULATION	±1.5%	±2.0%	±1.5%			
INPUT	SETUP, RISE TIME	300ms, 15ms/230VAC	300ms, 15ms/115VAC at full load				
	HOLD UP TIME (Typ.)	70ms/230VAC	14ms/115VAC at full load				
PROTECTION	VOLTAGE RANGE	90 ~ 264VAC	127 ~ 370VDC				
	FREQUENCY RANGE	47 ~ 63Hz					
	EFFICIENCY (Typ.)	78%	82%				
	AC CURRENT (Typ.)	1.1A/115VAC	0.7 A/230VAC				
	INRUSH CURRENT (Typ.)	COLD START 60A/230VAC	30A/115VAC				
ENVIRONMENT	LEAKAGE CURRENT Note.5	Earth leakage current < 150 μA/264VAC , Touch current < 100 μA/264VAC					
	OVERLOAD	115 ~ 150% rated output power Protection type : Hiccup mode, recovers automatically after fault condition is removed					
	OVER VOLTAGE	CH1: 5.75 ~ 6.75V Protection type : Shut down o/p voltage, re-power on to recover					
	WORKING TEMP.	-20 ~ +65°C (Refer to "Derating Curve")					
SAFETY & EMC (Note 9)	WORKING HUMIDITY	20 ~ 90% RH non-condensing					
	STORAGE TEMP., HUMIDITY	-40 ~ +85°C, 10 ~ 95% RH non-condensing					
	TEMP. COEFFICIENT	±0.03%/°C (0 ~ 45°C)					
	VIBRATION	10 ~ 500Hz, 2G 10min./1cycle, period for 60min. each along X, Y, Z axes					
	OPERATING ALTITUDE Note.6	3000 meters					
OTHERS	SAFETY STANDARDS	UL62368-1, TUV BS EN/EN62368-1, IEC62368-1, IEC60601-1, EAC TP TC 004, UL ANSI/AAMI ES60601-1, CAN/CSA-C22.2 No. 60601-1:14 - Edition 3 approved, TUV BS EN/EN60601-1 approved					
	ISOLATION LEVEL	Primary-Secondary: 2xMOPP, Primary-Earth:1xMOPP, Secondary-Earth:1xMOPP					
	WITHSTAND VOLTAGE	I/P-O/P:4KVAC I/P-FG:2KVAC O/P-FG:1.5KVAC					
	ISOLATION RESISTANCE	I/P-O/P, I/P-FG, O/P-FG:100M Ohms / 500VDC / 25°C / 70% RH					
	EMC EMISSION	Parameter	Standard	Test Level / Note			
		Conducted emission	BS EN/EN55011 (CISPR11)	Class B			
		Radiated emission	BS EN/EN55011 (CISPR11)	Class B			
		Harmonic current	BS EN/EN61000-3-2	Class A			
	EMC IMMUNITY	Voltage flicker	BS EN/EN61000-3-3	-----			
		BS EN/EN60601-1-2					
		Parameter	Standard	Test Level / Note			
		ESD	BS EN/EN61000-4-2	Level 4, 15KV air ; Level 4, 8KV contact			
		RF field susceptibility	BS EN/EN61000-4-3	Level 3, 10V/m(80MHz~2.7GHz) Table 9, 9~28V/m(385MHz~5.78GHz)			
		EFT bursts	BS EN/EN61000-4-4	Level 3, 2KV			
		Surge susceptibility	BS EN/EN61000-4-5	Level 4, 4KV/Line-FG ; 2KV/Line-Line			
		Conducted susceptibility	BS EN/EN61000-4-6	Level 3, 10V			
		Magnetic field immunity	BS EN/EN61000-4-8	Level 4, 30A/m			
		Voltage dip, interruption	BS EN/EN61000-4-11	100% dip 1 periods, 30% dip 25 periods, 100% interruptions 250 periods			
NOTE	MTBF	677.8K hrs min. MIL-HDBK-217F (25°C)					
	DIMENSION (L*W*H)	101.6*50.8*29mm or 4" * 2" * 1.14" inch					
	PACKING	0.15Kg; 96pcs/15.4Kg/0.89CUFT					
1. All parameters NOT specially mentioned are measured at 230VAC input, rated load and 25°C of ambient temperature. 2. 33% Duty cycle maximum within every 30 seconds. Average output power should not exceed the rated power. 3. Ripple & noise are measured at 20MHz of bandwidth by using a 12" twisted pair-wire terminated with a 0.1μf & 47μf parallel capacitor. 4. Tolerance : includes set up tolerance, line regulation and load regulation. 5. Touch current was measured from primary input to DC output. 6. The ambient temperature derating of 3.5°C/1000m with fanless models and of 5°C/1000m with fan models for operating altitude higher than 2000m(6500ft). 7. Length of set up time is measured at cold first start. Turning ON/OFF the power supply may lead to increase of the set up time. 8. Heat Sink HS1,HS2 can not be shorted. 9. The power supply is considered a component which will be installed into a final equipment. All the EMC tests are been executed by mounting the unit on a 360mm*360mm metal plate with 1mm of thickness. The final equipment must be re-confirmed that it still meets EMC directives. For guidance on how to perform these EMC tests, please refer to "EMI testing of component power supplies." (as available on http://www.meanwell.com)							
※ Product Liability Disclaimer : For detailed information, please refer to https://www.meanwell.com/serviceDisclaimer.aspx							




60W Reliable Dual Output Medical Grade

RPD-60 series


■ Block Diagram

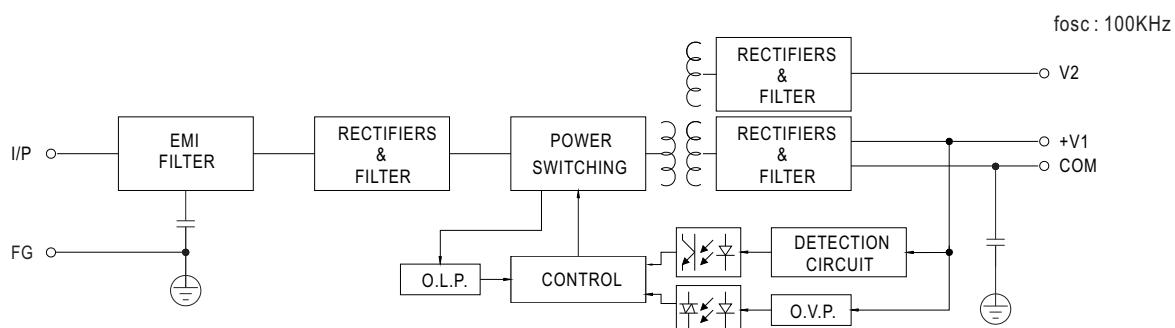


■ Derating Curve

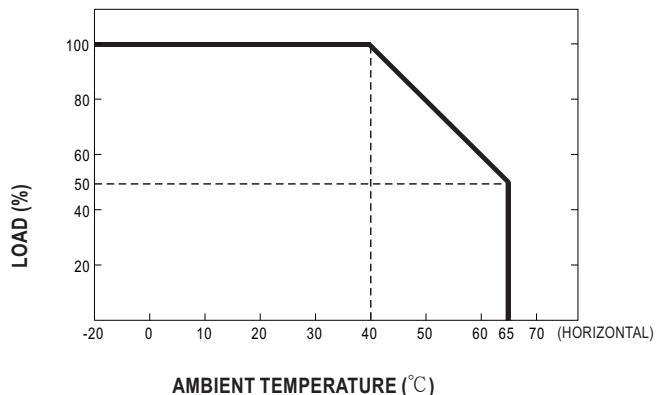

■ Output Derating VS Input Voltage

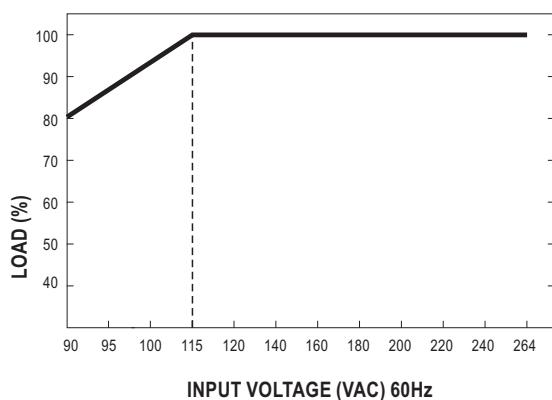

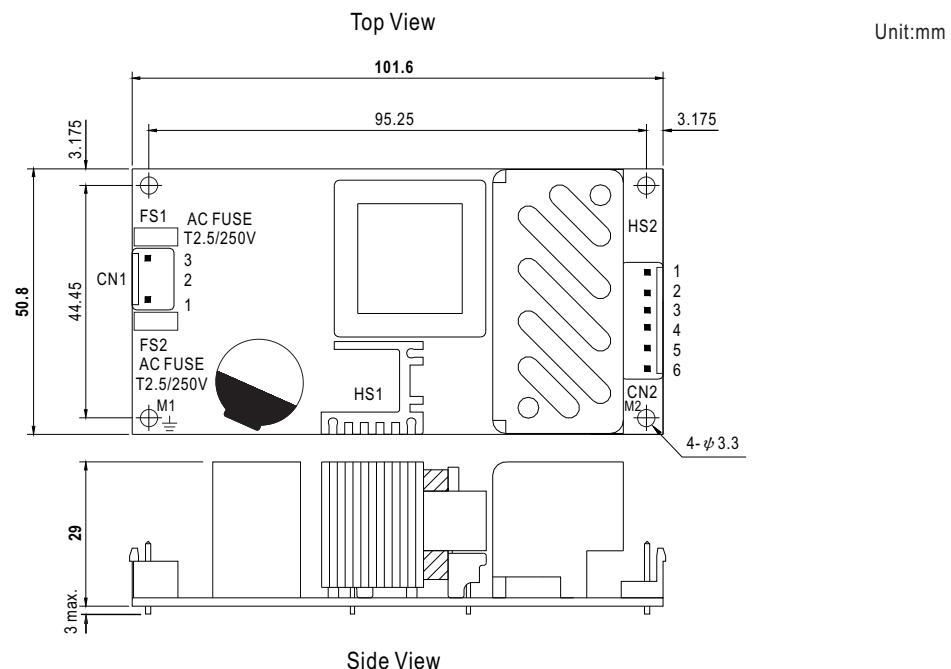Mechanical Specification

AC Input Connector (CN1) : JST B3P-VH or equivalent

Pin No.	Assignment	Mating Housing	Terminal
1	AC/N	JST VHR or equivalent	JST SVH-21T-P1.1 or equivalent
2	No Pin		
3	AC/L		

DC Output Connector (CN2) : JST B6P-VH or equivalent

Pin No.	Assignment	Mating Housing	Terminal
1,2	V1	JST VHR or equivalent	JST SVH-21T-P1.1 or equivalent
3,4	COM		
5	V2		
6	NC		

\pm : Grounding Required



- 1.HS1,HS2 cannot be shorted.
- 2.M1 is safety ground. For better EMC performance, Please secure an electrical connection between M1,M2 and chassis grounding.

Installation Manual

Please refer to : <http://www.meanwell.com/manual.html>